
CERTIFICATE OF CALIBRATION

ISSUED BY

Cirrus Research plc

DATE OF ISSUE 30 July 2021

CERTIFICATE NUMBER 160720

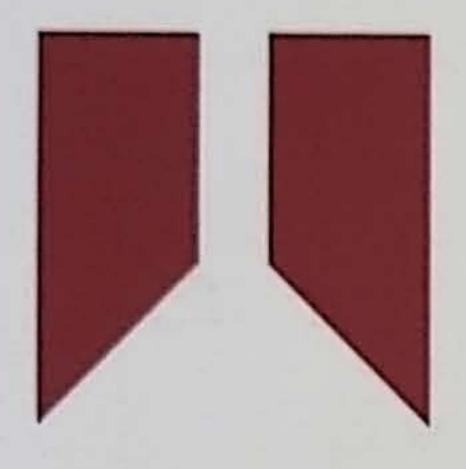

Cirrus Research plc **Acoustic House Bridlington Road** Hunmanby North Yorkshire YO14 0PH **United Kingdom**

Page 1 of 2

Approved signatory

T.Goodrich

Electronically signed:

Sound Level Meter: IEC 61672-3:2013

Instrument information

Manufacturer:

Cirrus Research plc

Notes:

Model:

CR:152B

Serial number:

G080495

Class:

Firmware version:

3.2.3197

Test summary

Date of calibration:

29 July 2021

The calibration was performed respecting the requirements of ISO/IEC 17025:2017. Periodic tests were performed in accordance with procedures from IEC 61672-3:2013.

The sound level meter submitted for testing successfully completed the class 2 periodic tests of IEC 61672-3:2013, for the environmental conditions under which the tests were performed.

However, no general statement or conclusion can be made about conformance of the sound level meter to the full specifications of IEC 61672-1:2013 because (a) evidence was not publicly available, from an independent testing organisation responsible for pattern approvals, to determine that the model of sound level meter fully conformed to the class 2 specifications in IEC 61672-1:2013 or correction data for acoustical test of frequency weighting were not provided in the Instruction Manual and (b) because the periodic tests of IEC 61672-3:2013 cover only a limited subset of the specifications in IEC 61672-1:2013.

Notes

This certificate provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory. The results within this certificate relate only to the items calibrated. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor k=2, providing a coverage probability of approximately 95%.